



Technical Note

Percutaneous femoral access: Stuck guide wire, decannulation difficulty due to unravelling and knotting

Bhanu Pratap Singh Chauhan, Binita Dholakia, Ashfaque Khan, Chirag Hirani, Satheesh Kumar, Dibya Jyoti Mahakul, Abhishek Katyal, Wajid Nazir, Daljit Singh

Department of Neurosurgery, GB Pant Institute of Post Graduate Medical Education and Research, New Delhi, India

J Cerebrovasc Endovasc Neurosurg.
March 27, 2024 [Epub ahead of print]

Received: 27 June 2023

Revised: 25 November 2023

Accepted: 20 December 2023

Correspondence to

Bhanu Pratap Singh Chauhan

Department of Neurosurgery, GB Pant Institute of Post Graduate Medical Education and Research, Jawaharlal Nehru Marg, New Delhi, India

Tel +91-9510-16-6157

E-mail bhanupratap1819@gmail.com

ORCID <https://orcid.org/0000-0001-8473-7453>

Percutaneous techniques for femoral arterial access are increasingly being performed due to advances in endovascular cerebral procedures, as they provide a less morbid and minimally invasive approach than open procedures. Common complications associated with this peripheral puncture include hematoma, bleeding, pseudoaneurysm, arteriovenous fistula, retroperitoneal bleeding, inadvertent venous puncture, dissection, etc. The retrograde femoral access is currently the most frequently used arterial access as it is technically straightforward, allows for the use of larger size sheaths and catheters, allows repeated attempts, etc. Although being technically less challenging, grave complications can occur due to hardware failure. Here, we present a case of unruptured posterior inferior cerebellar artery (PICA) aneurysm, who underwent uneventful diagnostic cerebral digital subtraction angiography (DSA) via right femoral artery route on first attempt, but on second attempt for therapeutic intervention, landed up with stuck guide wire and faced decannulation difficulty due to unravelling of guide wire and multiple knot formation, which was finally removed after multiple attempts at pulling and improvised manoeuvres. Such cannulation and decannulation difficulties have been reported multiple times for central venous access, but extremely rarely for femoral routes, making this case a rarity and worth reporting.

Keywords Percutaneous, Femoral, Access, Decannulation, Stuck, Guide wire

INTRODUCTION

Endovascular procedures are increasingly being used to treat various cerebrovascular disease entities like aneurysm, arteriovenous malformation, tumor embolization, stroke thrombolysis and thrombectomy, middle meningeal artery embolization for chronic subdural haemorrhage, carotid stenosis, cerebral venous thrombosis, dural fistulas, etc. Trans-femoral is considered as classical approach over trans-radial, and hence is increasingly being performed in contemporary times, allowing for

This is an Open Access article distributed under the terms of the Creative Commons Attribution Non-Commercial License (<http://creativecommons.org/licenses/by-nc/4.0/>) which permits unrestricted non-commercial use, distribution, and reproduction in any medium, provided the original work is properly cited.

unlimited repetition of puncturing, easy access, less radiation time and less contrast usage.¹⁾ Complications include hematoma, bleeding, pseudoaneurysms, fistulas, retroperitoneal haemorrhage, venous puncture, dissection, etc. and they have been well reported, when the puncture is inappropriate.⁵⁾ However, among rarely reported complications due to hardware failure owing to intraluminal knotting, unravelling, most of them have been for central venous cannulation, specifically for subclavian vein, most likely due to curved path of the vein over first rib.³⁾⁴⁾ Such complications while cannulating and decannulating the femoral artery are scarcely reported.

ILLUSTRATIVE CASE

A 55 year old, moderately built female, on presenting with headache, was diagnosed with unruptured right proximal posterior inferior cerebellar artery (PICA) aneurysm (Fig. 1) by diagnostic cerebral digital subtraction angiography (DSA), which was uneventfully accomplished by right femoral artery access in first attempt with smooth cannulation via single wall Seldinger technique. Subsequently, after 2 days, she was taken up for



Fig. 1. Cerebral DSA selective shoot of right vertebral artery showing right proximal PICA aneurysm. DSA, digital subtraction angiography; PICA, posterior inferior cerebellar artery

therapeutic intervention by endovascular coiling, for which again percutaneous right femoral access was planned by manual palpatory method, via entry point 1.5 cm below the mid inguinal point. After initial puncture with single wall Seldinger technique using 18G puncture needle, guide wire (diameter 0.038", length 45 cm, J tip) was introduced, which went through with little resistance. Puncture needle was removed, and 7F introducer sheath was threaded over the wire as standard practice, after placing the nick on skin and subcutaneous tissue. On attempting to withdraw the wire with introducer sheath, significant resistance was encountered, resulting in failure of removal. Immediately, puncture site was visualised under fluoroscopy guidance, and guide wire was found to be bent, with an inferiorly directed loop in the femoral artery (Fig. 2A). However, position of introducer sheath was confirmed in the lumen by good back flow of blood from the side channel. Multiple attempts were made to remove the wire by to and fro movement, by pushing it to straighten it, by pulling it against resistance, but everything failed. Instead of straightening, the wire looped several times (Fig. 2B). Next, an attempt was made to pass a 5 French multipurpose catheter (MPC) over the wire through the diaphragm of the check flow, which could only be negotiated till the first bend of wire (Fig. 2C). The discrepancy in the length of MPC (90 cm), over the wire (45 cm), was resolved by cutting the MPC, till proximal part of guide wire was visualised. Introducer sheath was withdrawn, and attempt was made to remove the entire assembly en masse, which also failed. Cardiothoracic and Vascular surgeons' team was summoned for help and planned for arteriotomy and removal, during which, after removal of MPC, it was noticed that distal guide wire was broken and had gotten separated into rigid straight central core and overlying soft coiled part which became unravelled (Fig. 2D). On final attempt by grasping the rigid core wire, using improvised rotational manoeuvre simultaneously with pulling, the proximal end got dislodged and retrieval was successful. Immediately the access site was compressed manually, after haemostasis was ensured, good femoral and dorsalis pedis pulsations

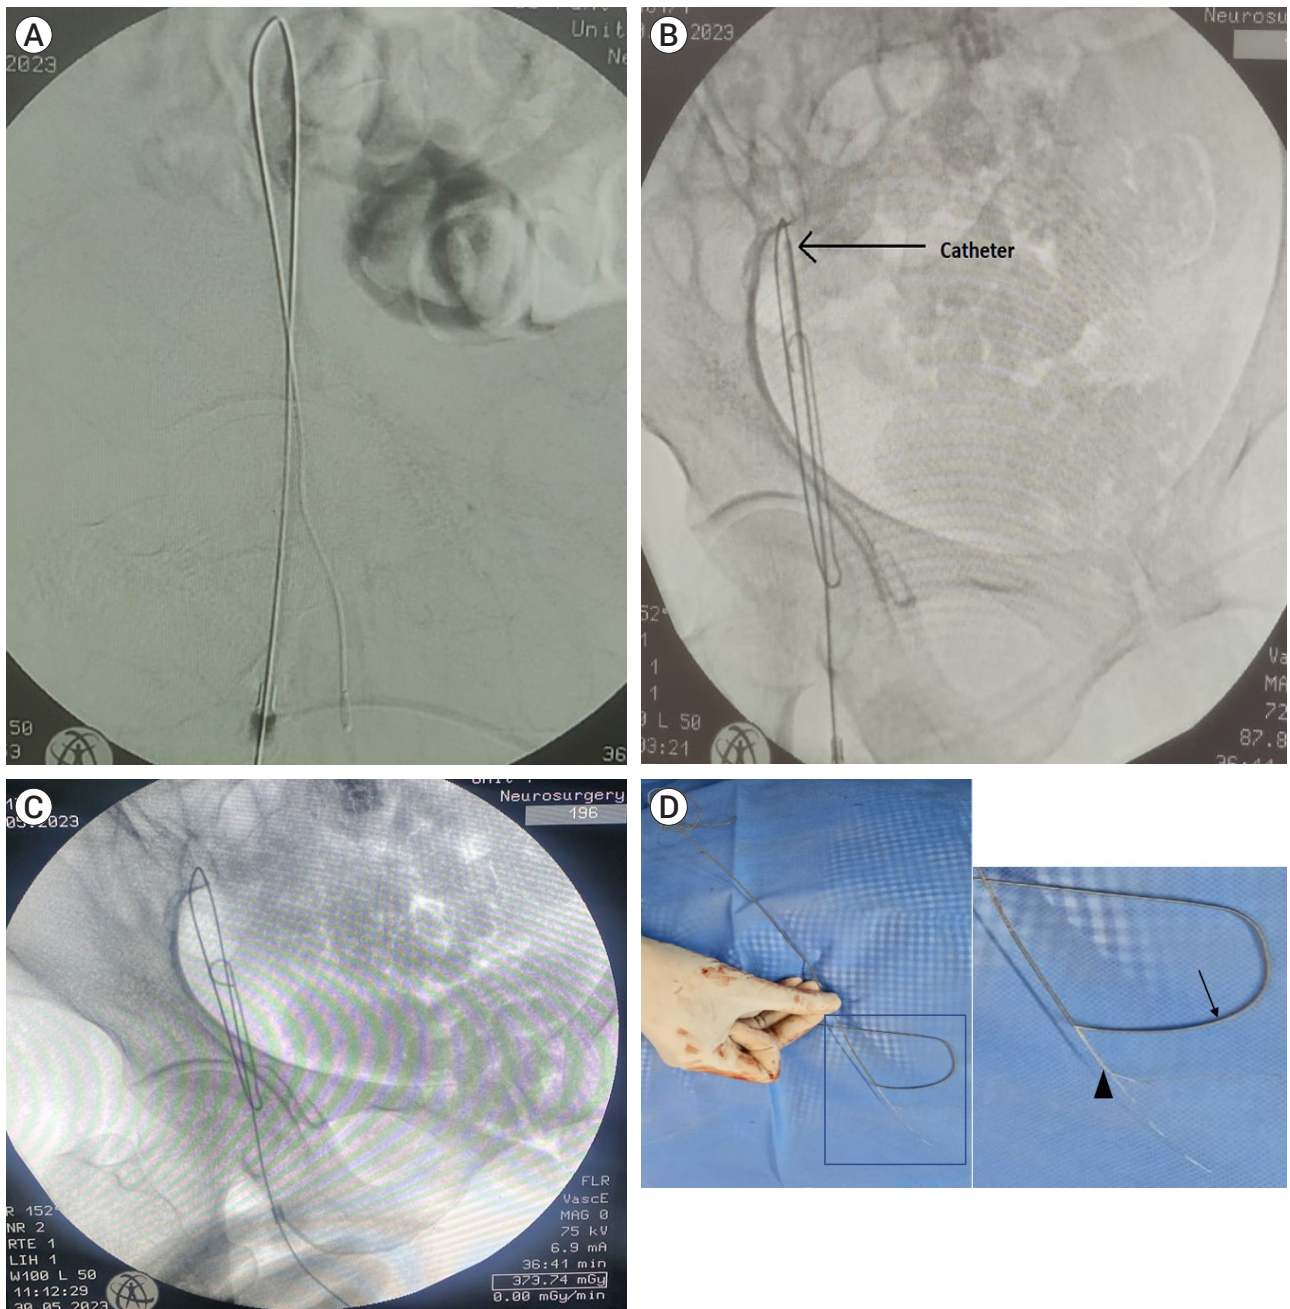


Fig. 2. (A) Fluoroscopic image showing check flow with guide wire, and its inferiorly directed loop in the femoral artery. (B) Fluoroscopic image showing multiple loops and knotting of guide wire in the common femoral artery. (C) Fluoroscopic image showing MPC (catheter) negotiated upto the first bend, couldn't be negotiated any further, and failed to straighten the wire. (D) Image showing distal end has separated into rigid central core (arrow head) and overlying soft part (arrow), which has unraveled (box magnified view). Multiple loops formed by the unraveled soft part seen in the proximal end after removal. MPC, multipurpose catheter

were palpable. The coiling of aneurysm was then completed successfully via left femoral artery puncture and patient was discharged uneventfully.

DISCUSSION

Intravascular knot formation, unravelling, knotting and kinking of guide wire is common for central venous

cannulations, literature regarding knot formation while cannulating the artery in one attempt is scarce, and retrieval of such kinked and unravelled wire, without major morbid complications is even scarcer.²⁾ Here, the suspected causes are speculated to be overly malleable and faulty guide wire, inadequate nick over skin and subcutaneous tissue leading to introducer sheath tip damage due to forceful insertion against resistance (damaged tip can damage the wire as well as intima during manipulation), repeated attempt via the same side within short interval, and forceful introduction of wire against even slight resistance. One must exert extreme caution while selecting the entry point, and inspect the hardware minutely before the procedure, and keep extremely low threshold for resistance and manoeuvring difficulties, to avoid such incidents.

CONCLUSIONS

Complications like these are extremely uncommon and their unpredictability makes them difficult to manage. Before attempting forceful introduction or removal of guide wire, the target site should be visualised under fluoroscopic guidance to confirm the point of resistance and status of guide wire in the lumen.

Disclosure

The authors report no conflict of interest concerning the materials or methods used in this study or the findings specified in this paper.

REFERENCES

1. Anjum I, Khan MA, Aadil M, Faraz A, Farooqui M, Hashmi A. Transradial vs. Transfemoral approach in cardiac catheterization: A literature review. *Cureus*. 2017 Jun;9(6):e1309.
2. Barik AK, Gupta P, Andleeb R, Chaturvedi J. Retrieval of self-knotted and unraveled guide wire in the femoral artery: Focus on point-of-care ultrasound (POCUS). *Curr Med Res Pr*. 2019;9(6):249-50.
3. Jalwal GK, Rajagopalan V, Bindra A, Rath GP, Goyal K, Kumar A, et al. Percutaneous retrieval of malpositioned, kinked and unraveled guide wire under fluoroscopic guidance during central venous cannulation. *J Anaesthesiol Clin Pharmacol*. 2014 Apr;30(2):267-9.
4. Khan KZ, Graham D, Ermenyi A, Pillay WR. Case report: Managing a knotted Seldinger wire in the subclavian vein during central venous cannulation. *Can J Anaesth*. 2007 May; 54(5):375-9.
5. Ndrepepa G, Berger PB, Mehilli J, Seyfarth M, Neumann FJ, Schömig A, et al. Periprocedural bleeding and 1 year outcome after percutaneous coronary intervention: Appropriateness of including bleeding as a component of a quadruple end point. *J Am Coll Cardiol*. 2008 Feb;51(7):690-7.